

MARK 8 OZONE MACHINE

***Capable of 5 days and nights(125 hours) for ozonated glycerine**



***Not for sale or resale. Only for the use by IAOS trained medical personal only**



info@iaos.org.in
iaos.org.in@gmail.com



www.iaos.org.in



[+91 9791020615](tel:+919791020615)
(No calls, Whatsapp only)

The lesser known miracle molecule in modern medicine



Each machine is individually calibrated and certified accurate.

First annual calibration free.

One year warranty.

First indian CE certified medical ozone machine.

EC DIRECTIVE CE MARK



Certificate of Registration
EC DIRECTIVE CE MARK

Certificate No. 17802

This is to certify that the Technical Documentation for the
IAOS EBOO system
IAOS MARK 6A MARK 8, MARK 9 &
MARK 10 MEDICAL OZONE MACHINE
MARK 2, 3, 4 MEDICAL HYDROGEN GENERATING MACHINE

manufactured by
IAOS TECHNOLOGY PRIVATE LIMITED
29, Karuneeagar street, Nerkundram, Chennai-60007, Tamilnadu.

has been found to conform to:
EN 61000-3-3:2013, EN 61000-3-2:2014
EN 55014-2:2015, EN 55014-1:2016

The Certificate is valid for the products mentioned above
Based on our review we can confirm that the technical file for the products
mentioned above meets the requirements of the relevant EC Directives
the Manufacturer is responsible for certifying the product and ensuring that all manufactured
products are in compliance with the specification detailed in the technical construction file

Date of Registration: 01/11/2025
Date of Expiry: 31/10/2028
Re-certification Date: 31/10/2028
Signed on behalf of AQSR




American Quality Standards Registrars,
A 1203 Green olive apartment Hinjewadi 411057 Maharashtra India Web. www.aqsrworld.com

Any significant changes in the design or construction of products, the quality system or amendments to the Directive may render the certificate invalid at an earlier date. ☐e product liability rests with the manufacturer in accordance with the European Council Directives.





Power supply

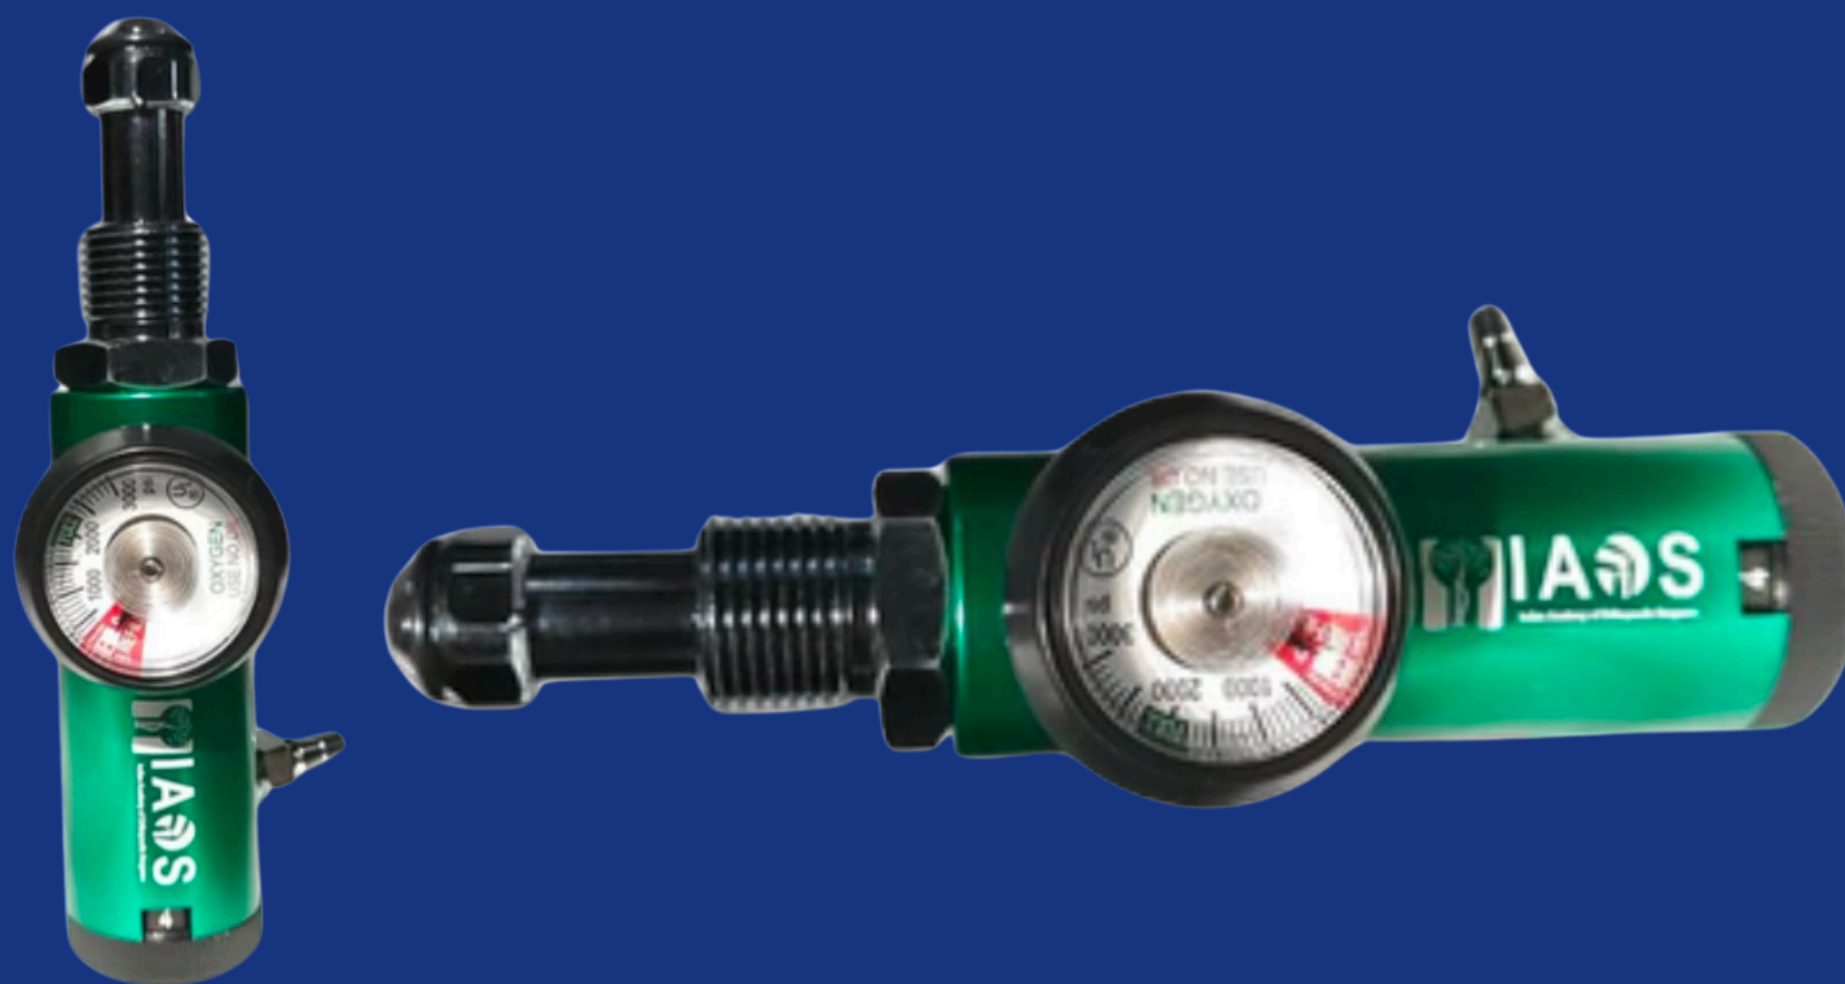

**Special regulator with up to 1/32
of litre regulator**






Silicon Tubings







Connectors

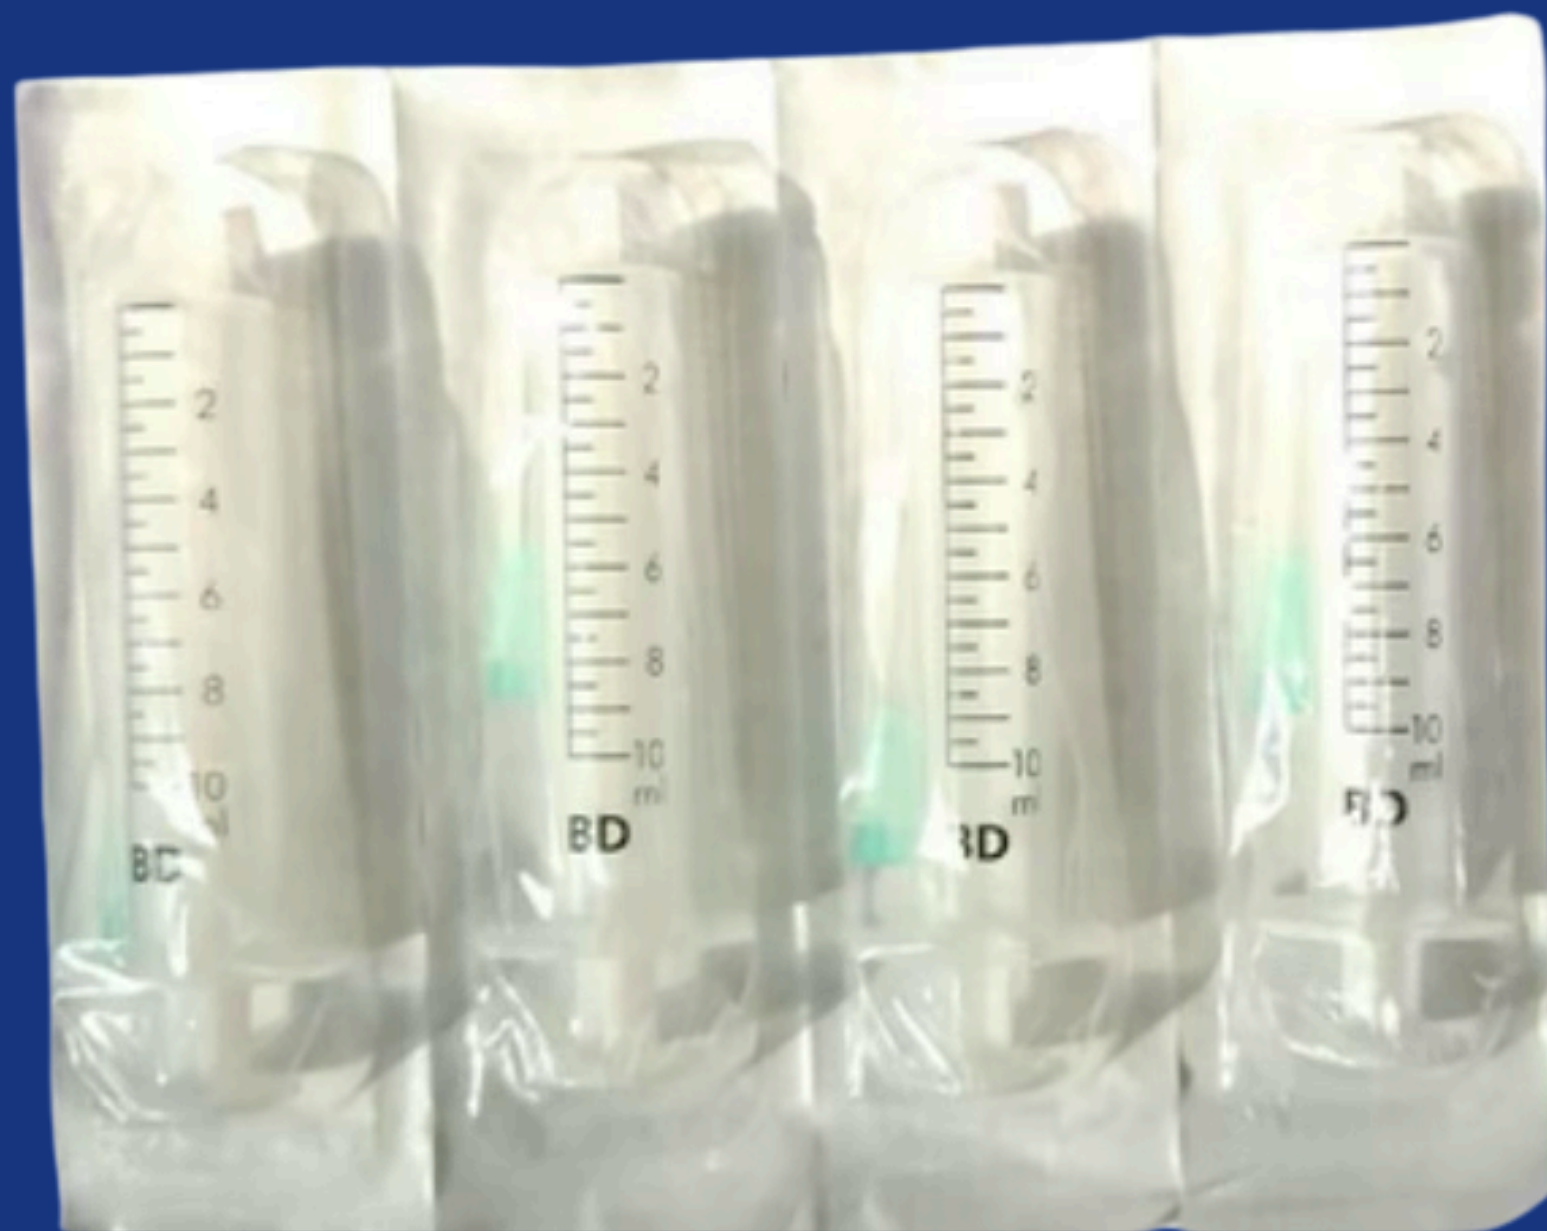

10 CC latex free syringes



20 CC latex free syringes

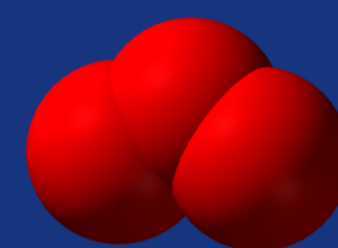
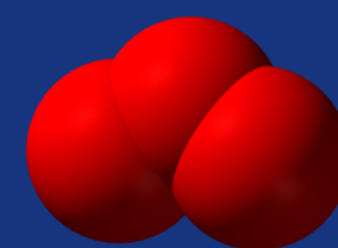
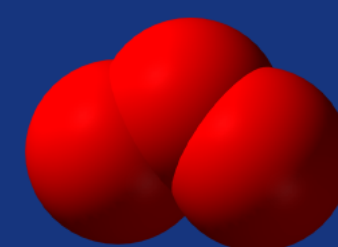
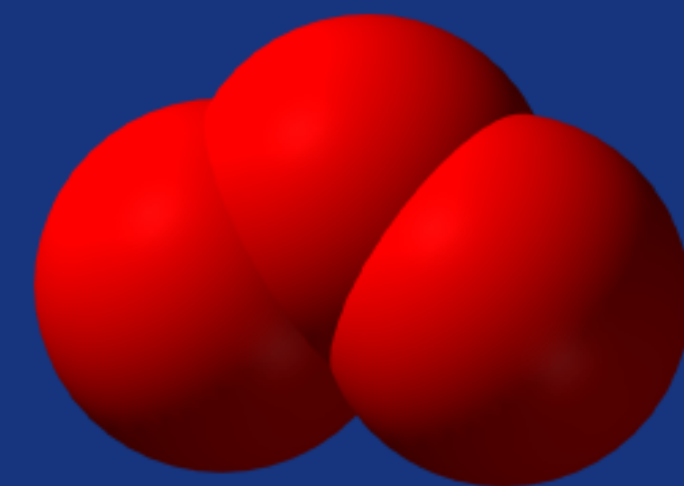





50 CC latex free syringes



ozone wound bags

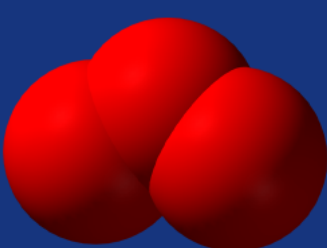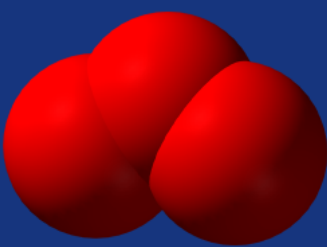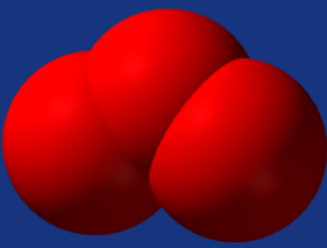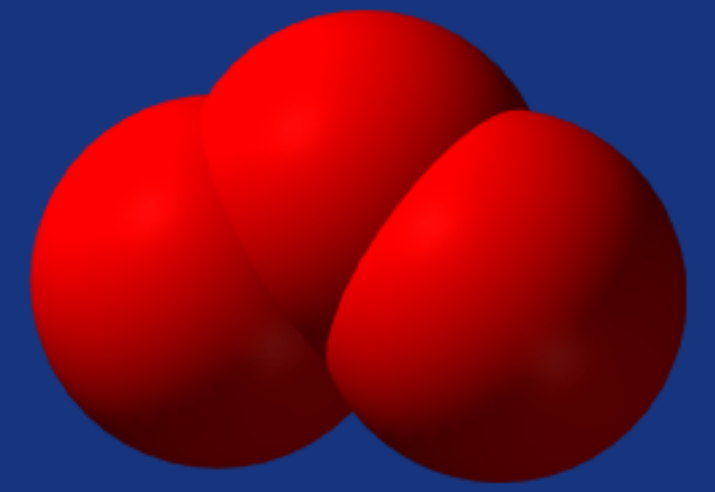

Diffuser stones

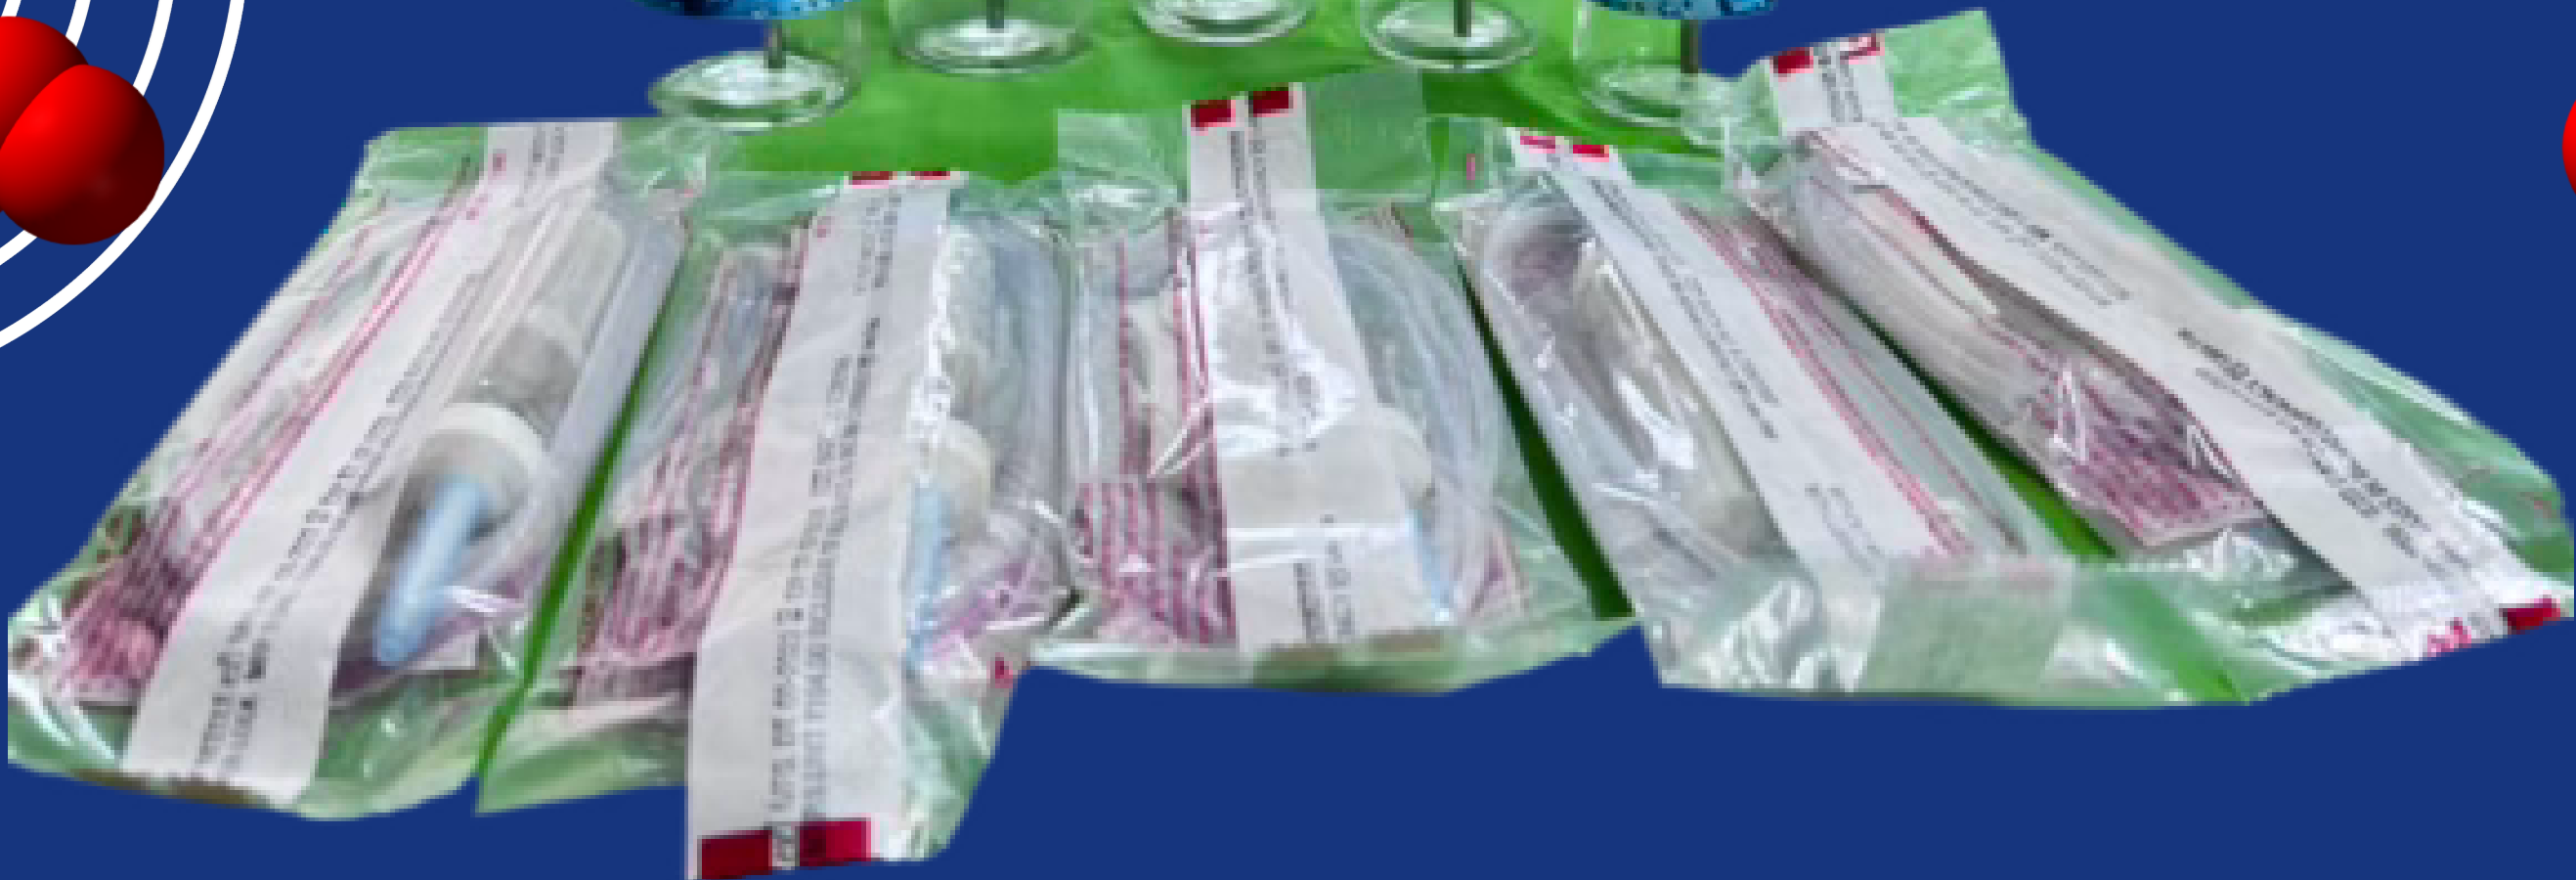


MAHT Vacuum bottles with special transfusion sets

Flexible schedule molecular therapy course with lectures, lessons and videos.

32 modules


Certificate will be provided on completion of course

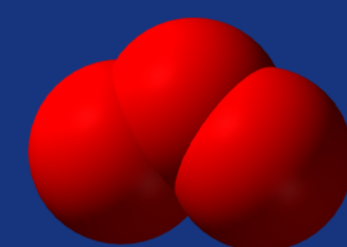


3 to 4 months Fellowship/Certification course by OMTA/GAMT.

PDF files of 32 lectures and 32 lessons.

32 detailed video lectures of one hour or more and renowned Scientifically structured valuable teaching programme.

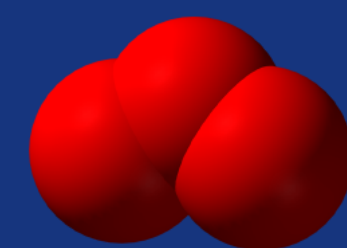

Nationally internationally faculty.

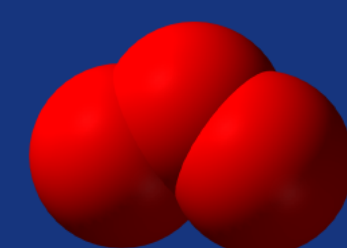



O.M.T.A

OZONE AND MOLECULAR THERAPIES ASSOCIATION



GLOBAL ACADEMY OF MOLECULAR THERAPEUTICS



*Certification for four months Fellowship/ Course in
Molecular therapeutics and Ozone Therapy*

This Certifies that

Dr. Xxxx

*has completed the above Fellowship/course held between
November 2024 to February of 2025*

Dr Prasham Shah


PRESIDENT

March 1st 2025

Dr Aroop Mukharjee


VICE PRESIDENT

**Certification from GAMT/OMTA
at the end of the course.**

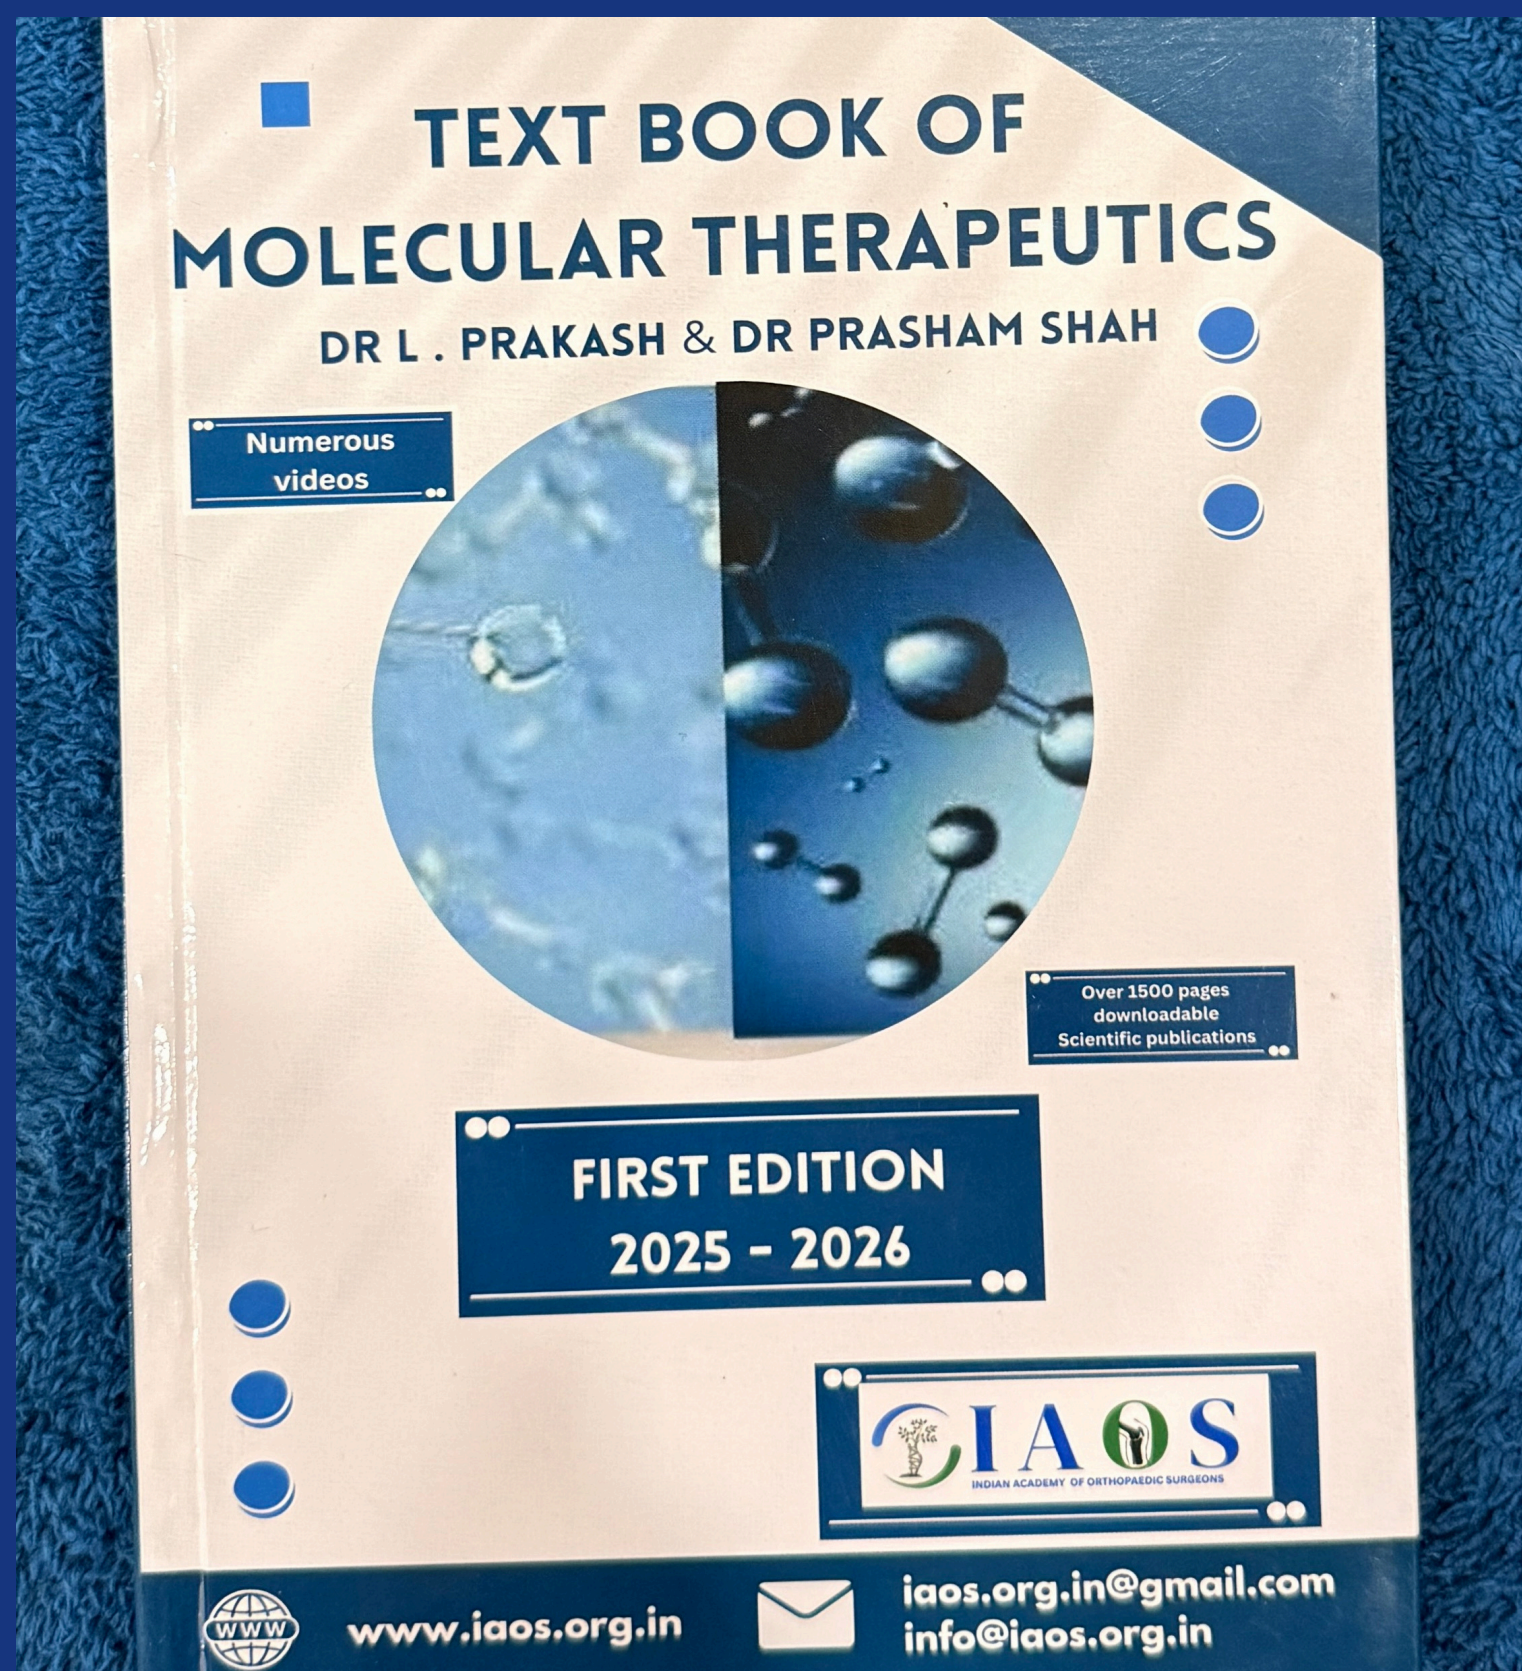

Hard Bound Book





Account Details:

Account No:120001617498

Name: IAOS Technology Private Limited

Bank Name : Canara Bank

IFSC Code: Cnrb0001166

IAOS TECHNOLOGY PRIVATE LIMITED



311632119617498@cnrb

**Retail Price
Rs 1,75,000/-
GST 5%**

Share a screenshot of payment with your name and designation to +91 9791020615 WhatsApp. This is very important for you to be included to the WhatsApp group for participants.

You will receive the first set of study material in the form of high quality pdf files and lecture link in WhatsApp. Please ensure that you have a valid WhatsApp account to receive the files and links.



info@iaos.org.in
iaos.org.in@gmail.com



www.iaos.org.in



+91 9791020615
(No calls, Whatsapp only)